



20160814T122505Z – mixed Convection – Roughness=3.00mm; T=22.2+10.7°C; –90.00°
k=0.0258, Ra/L^3=1.010x10^9, h=5.20W/(K.m^2), U=0.483W/K, Nu=61.5, Pr=0.709

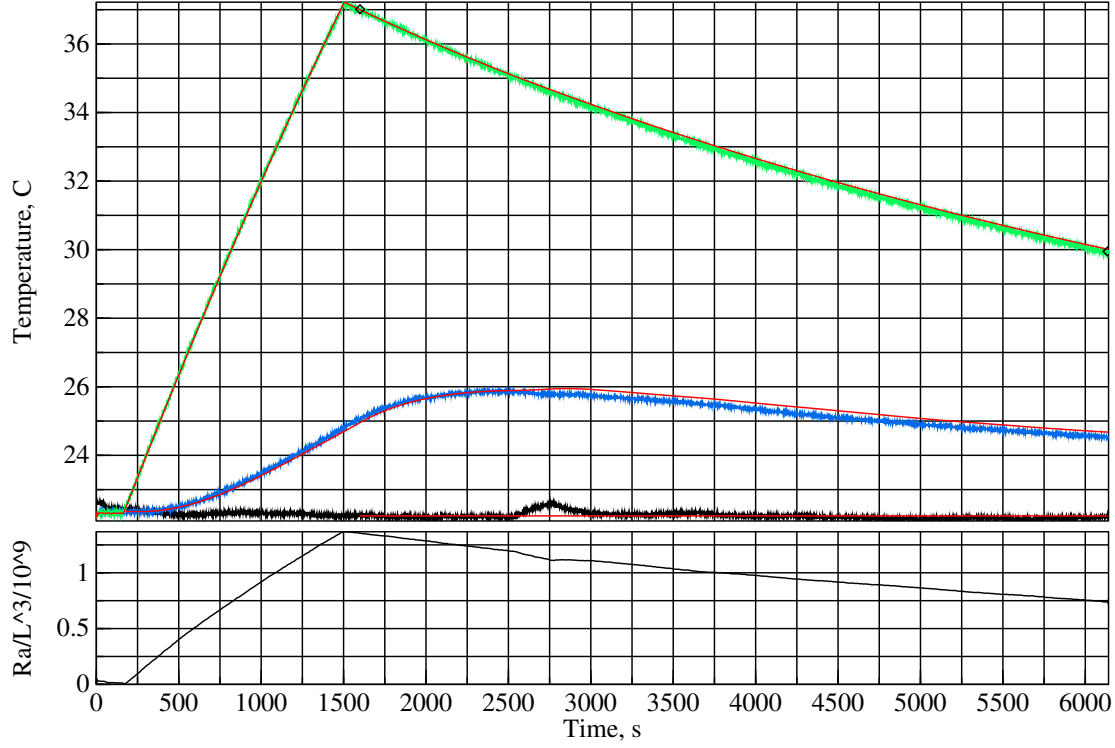

Estimated measurement uncertainties of natural convection at $\theta = -90.0$.

Symbol	Nominal	Sensitivity	Bias	Uncertainty	Component
ΔT	10.7K	+15.2%/K	0.10K	1.52%	LM35C differential
P	100kPa	+0.0005%/Pa	1.5kPa	0.78%	MPXH6115A6U air pressure
C_{pt}	4.69kJ/K	+0.029%/(J/K)	47J/K	1.37%	plate thermal capacity
C_S	1.000	–38.7%	0.050	1.94%	side reuptake
C_B	1.000	–10.6%	0.100	1.06%	back reuptake
L_c	0.305m	+421%/m	500um	0.21%	characteristic length
L_m	3.57mm	+828%/m	500um	0.41%	side metal strip width
ϵ_{XPS}	0.515	+25.1%	0.010	0.25%	XPS emissivity
ϵ_{tp}	0.890	+30.3%	0.015	0.45%	tape emissivity
Ω_{tp}	0.540	+20.5%	0.020	0.41%	tape coverage
ϵ_{rs}	0.040	+109%	0.010	1.09%	test-surface emissivity
ϵ_{wt}	0.900	+49.2%	0.025	1.23%	wind-tunnel emissivity
				3.61%	combined bias uncertainty


20160813T235139Z – mixed Convection – Roughness=3.00mm; T=22.6+10.6°C; –90.00°
40±2.5r/min, V=0.14m/s, Re=2880, Ra/L^3=0.993x10^9, h=5.14W/(K.m^2), U=0.478W/K, Nu=60.7

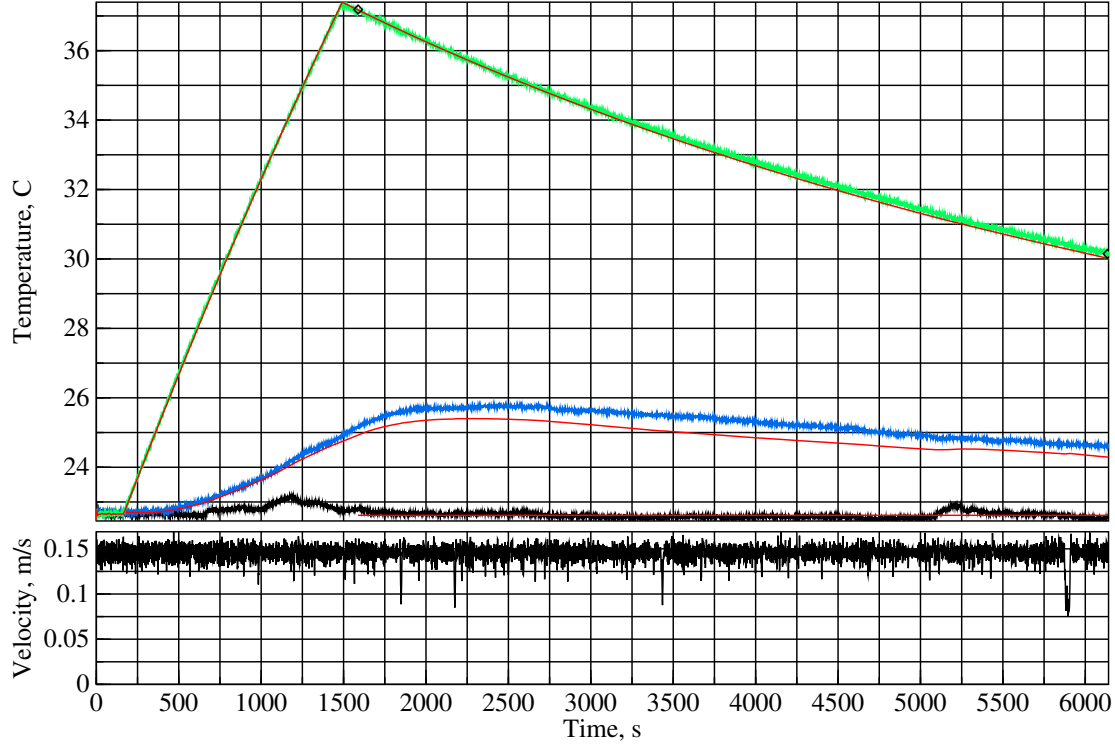

Estimated measurement uncertainties, bi-level 3mm roughness at $Re = 2880$.


Symbol	Nominal	Sensitivity	Bias	Uncertainty	Component
ΔT	10.6K	+15.0%/K	0.10K	1.50%	LM35C differential
P	101kPa	+0.0006%/Pa	1.5kPa	0.86%	MPXH6115A6U air pressure
C_{pt}	4.69kJ/K	+0.029%/(J/K)	47J/K	1.35%	plate thermal capacity
η	0.409	+28.1%	0.014	0.40%	anemometer calibration
C_S	1.000	–36.5%	0.050	1.83%	side reuptake
C_B	1.000	–11.2%	0.100	1.12%	back reuptake
L_c	0.305m	+401%/m	500um	0.20%	characteristic length
L_m	3.57mm	+843%/m	500um	0.42%	side metal strip width
ϵ_{XPS}	0.515	+23.8%	0.010	0.24%	XPS emissivity
ϵ_{tp}	0.890	+28.8%	0.015	0.43%	tape emissivity
Ω_{tp}	0.540	+19.4%	0.020	0.39%	tape coverage
ϵ_{rs}	0.040	+104%	0.010	1.04%	test-surface emissivity
ϵ_{wt}	0.900	+46.7%	0.025	1.17%	wind-tunnel emissivity
				3.56%	combined bias uncertainty
Symbol	Nominal	Sensitivity	Variability	Uncertainty	Component
ω	39.9r/min	+0.288%/(r/min)	2.5r/min	0.73%	fan rotation rate
				3.85%	RSS combined uncertainty

20160814T171610Z – mixed Convection – Roughness=3.00mm; T=20.9+10.6°C; -90.00°
55±2.9r/min, V=0.20m/s, Re=4009, Ra/L^3=1.016x10^9, h=5.47W/(K.m^2), U=0.509W/K, Nu=64.9

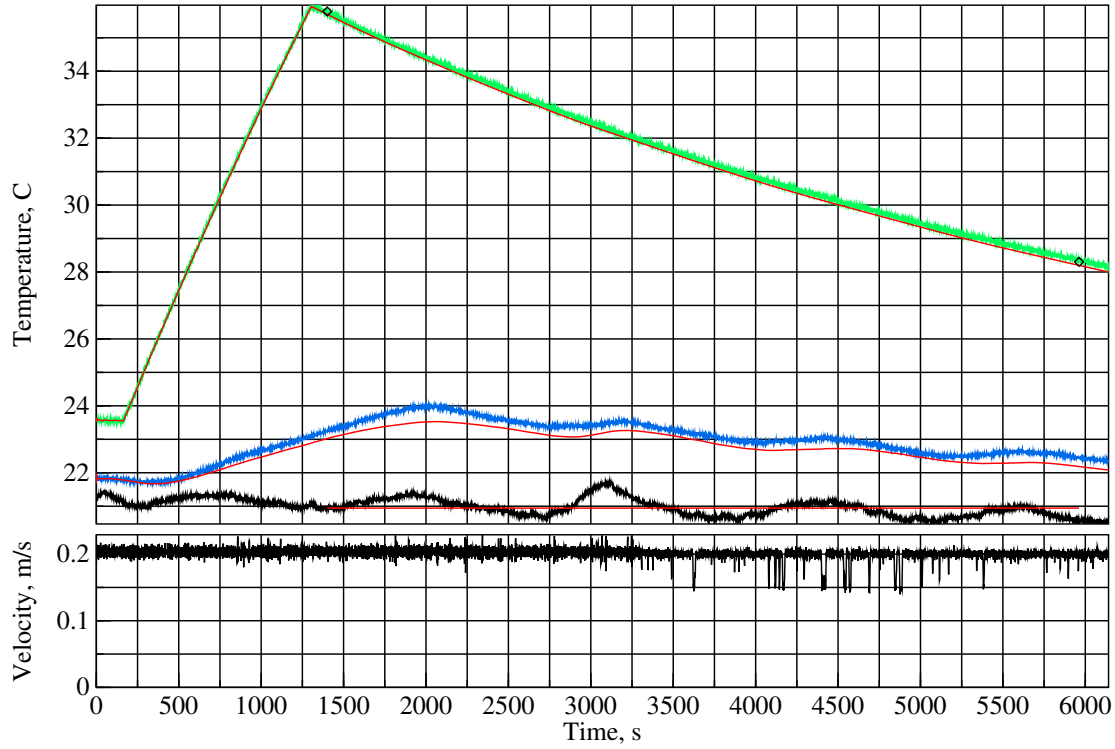

Estimated measurement uncertainties, bi-level 3mm roughness at $Re = 4008$.


Symbol	Nominal	Sensitivity	Bias	Uncertainty	Component
ΔT	10.6K	+14.6%/K	0.10K	1.46%	LM35C differential
P	100kPa	+0.0006%/Pa	1.5kPa	0.92%	MPXH6115A6U air pressure
C_{pt}	4.69kJ/K	+0.028%/(J/K)	47J/K	1.33%	plate thermal capacity
η	0.409	+48.1%	0.014	0.69%	anemometer calibration
C_S	1.000	-34.8%	0.050	1.74%	side reuptake
C_B	1.000	-11.1%	0.100	1.11%	back reuptake
L_m	3.57mm	+818%/m	500um	0.41%	side metal strip width
ϵ_{XPS}	0.515	+22.2%	0.010	0.22%	XPS emissivity
ϵ_{tp}	0.890	+26.8%	0.015	0.40%	tape emissivity
Ω_{tp}	0.540	+18.1%	0.020	0.36%	tape coverage
ϵ_{rs}	0.040	+97.1%	0.010	0.97%	test-surface emissivity
ϵ_{wt}	0.900	+43.5%	0.025	1.09%	wind-tunnel emissivity
				3.49%	combined bias uncertainty
Symbol	Nominal	Sensitivity	Variability	Uncertainty	Component
ω	55.1r/min	+0.358%/(r/min)	2.9r/min	1.02%	fan rotation rate
				4.05%	RSS combined uncertainty

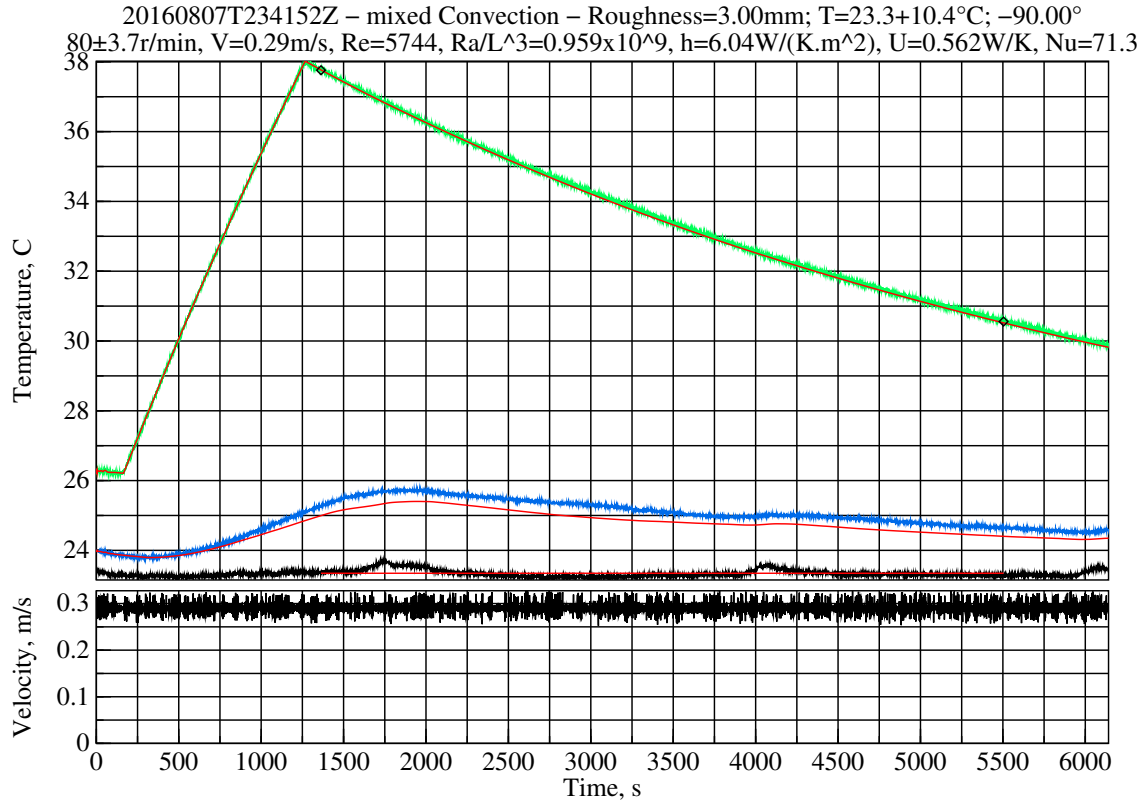

Estimated measurement uncertainties, bi-level 3mm roughness at $Re = 5744$.

Symbol	Nominal	Sensitivity	Bias	Uncertainty	Component
ΔT	10.4K	+14.4%/K	0.10K	1.44%	LM35C differential
P	100kPa	+0.0007%/Pa	1.5kPa	1.02%	MPXH6115A6U air pressure
C_{pt}	4.69kJ/K	+0.028%/(J/K)	47J/K	1.31%	plate thermal capacity
η	0.409	+83.3%	0.014	1.19%	anemometer calibration
C_S	1.000	-31.7%	0.050	1.58%	side reuptake
C_B	1.000	-10.6%	0.100	1.06%	back reuptake
ς	6.00mm	+2405%/m	100um	0.24%	post height
L_m	3.57mm	+802%/m	500um	0.40%	side metal strip width
ϵ_{XPS}	0.515	+20.8%	0.010	0.21%	XPS emissivity
ϵ_{tp}	0.890	+25.2%	0.015	0.38%	tape emissivity
Ω_{tp}	0.540	+17.0%	0.020	0.34%	tape coverage
ϵ_{rs}	0.040	+90.9%	0.010	0.91%	test-surface emissivity
ϵ_{wt}	0.900	+40.9%	0.025	1.02%	wind-tunnel emissivity
				3.51%	combined bias uncertainty
Symbol	Nominal	Sensitivity	Variability	Uncertainty	Component
ω	80.1r/min	+0.426%/(r/min)	3.7r/min	1.56%	fan rotation rate
				4.70%	RSS combined uncertainty


20160808T022413Z – mixed Convection – Roughness=3.00mm; T=23.4+10.5°C; –90.00°
160±3.4r/min, V=0.58m/s, Re=11470, Ra/L^3=0.970x10^9, h=9.02W/(K.m^2), U=0.839W/K, Nu=106.4

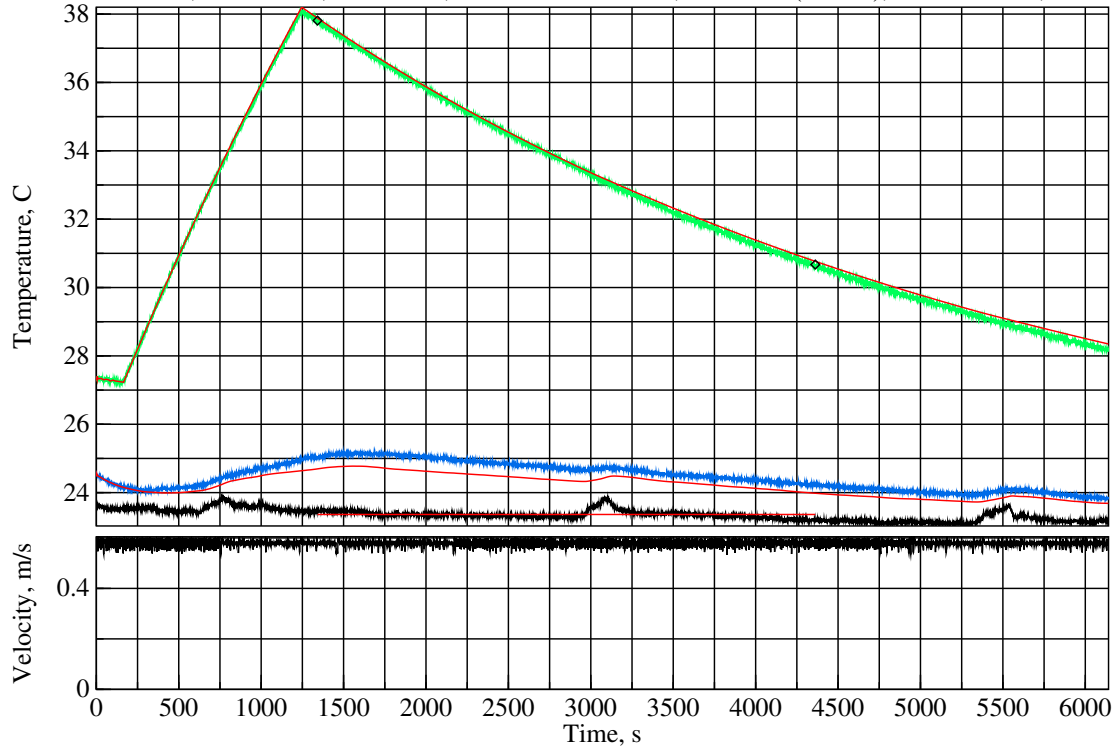

Estimated measurement uncertainties, bi-level 3mm roughness at $Re = 11470$.

Symbol	Nominal	Sensitivity	Bias	Uncertainty	Component
ΔT	10.5K	+12.6%/K	0.10K	1.26%	LM35C differential
P	101kPa	+0.0008%/Pa	1.5kPa	1.26%	MPXH6115A6U air pressure
C_{pt}	4.69kJ/K	+0.026%/(J/K)	47J/K	1.22%	plate thermal capacity
η	0.409	+167%	0.014	2.39%	anemometer calibration
C_S	1.000	–22.4%	0.050	1.12%	side reuptake
C_B	1.000	–7.87%	0.100	0.79%	back reuptake
ς	6.00mm	+4864%/m	100um	0.49%	post height
L_m	3.57mm	+657%/m	500um	0.33%	side metal strip width
ϵ_{tp}	0.890	+17.7%	0.015	0.27%	tape emissivity
Ω_{tp}	0.540	+11.9%	0.020	0.24%	tape coverage
ϵ_{rs}	0.040	+64.1%	0.010	0.64%	test-surface emissivity
ϵ_{wt}	0.900	+28.7%	0.025	0.72%	wind-tunnel emissivity
				3.70%	combined bias uncertainty
Symbol	Nominal	Sensitivity	Variability	Uncertainty	Component
ω	160r/min	+0.426%/(r/min)	3.4r/min	1.45%	fan rotation rate
				4.71%	RSS combined uncertainty


20160808T224235Z – mixed Convection – Roughness=3.00mm; T=22.7+10.4°C; –90.00°
320±2.4r/min, V=1.1m/s, Re=22910, Ra/L^3=0.984x10^9, h=16.0W/(K.m^2), U=1.48W/K, Nu=188.6

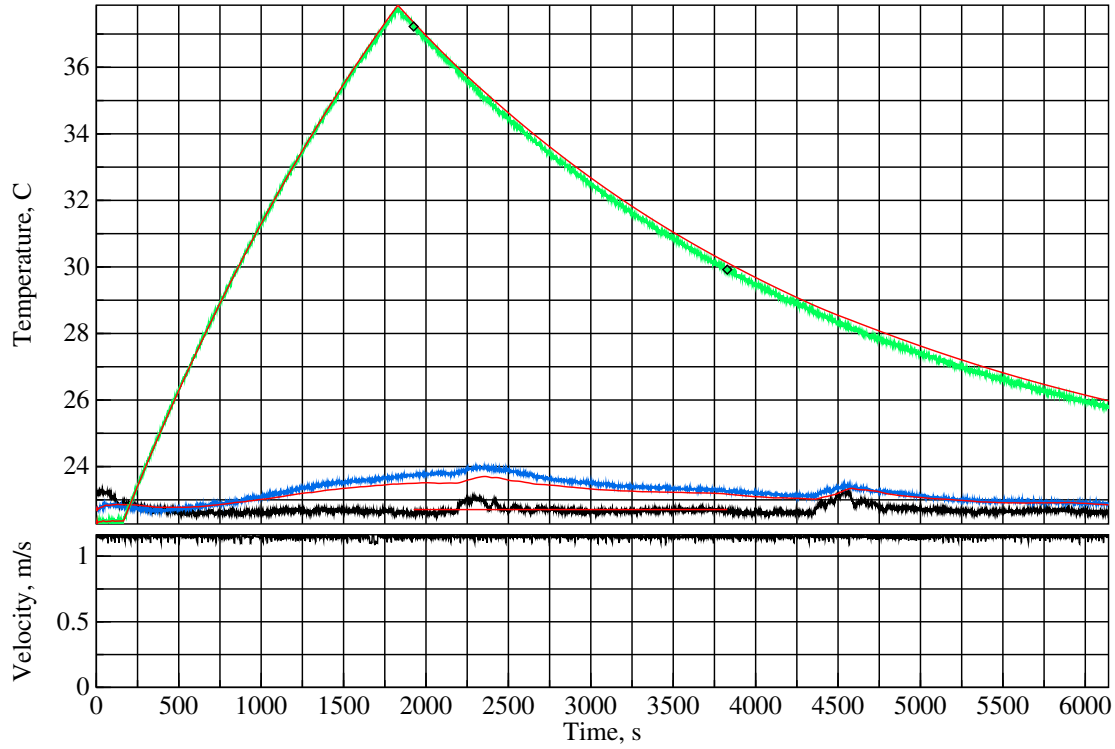

Estimated measurement uncertainties, bi-level 3mm roughness at $Re = 22910$.

Symbol	Nominal	Sensitivity	Bias	Uncertainty	Component
ΔT	10.4K	+11.1%/K	0.10K	1.11%	LM35C differential
P	101kPa	+0.0009%/Pa	1.5kPa	1.42%	MPXH6115A6U air pressure
C_{pt}	4.69kJ/K	+0.024%/(J/K)	47J/K	1.13%	plate thermal capacity
η	0.409	+220%	0.014	3.16%	anemometer calibration
C_S	1.000	–12.7%	0.050	0.64%	side reuptake
C_B	1.000	–4.64%	0.100	0.46%	back reuptake
ς	6.00mm	+6637%/m	100um	0.66%	post height
L_m	3.57mm	+476%/m	500um	0.24%	side metal strip width
ϵ_{rs}	0.040	+36.2%	0.010	0.36%	test-surface emissivity
ϵ_{wt}	0.900	+16.1%	0.025	0.40%	wind-tunnel emissivity
				4.00%	combined bias uncertainty
Symbol	Nominal	Sensitivity	Variability	Uncertainty	Component
ω	320r/min	+0.282%/(r/min)	2.4r/min	0.68%	fan rotation rate
				4.23%	RSS combined uncertainty


20160811T002147Z – mixed Convection – Roughness=3.00mm; T=22.8+10.1°C; -90.00°
640±4.8r/min, V=2.2m/s, Re=44534, Ra/L^3=0.955x10^9, h=27.5W/(K.m^2), U=2.56W/K, Nu=325.4

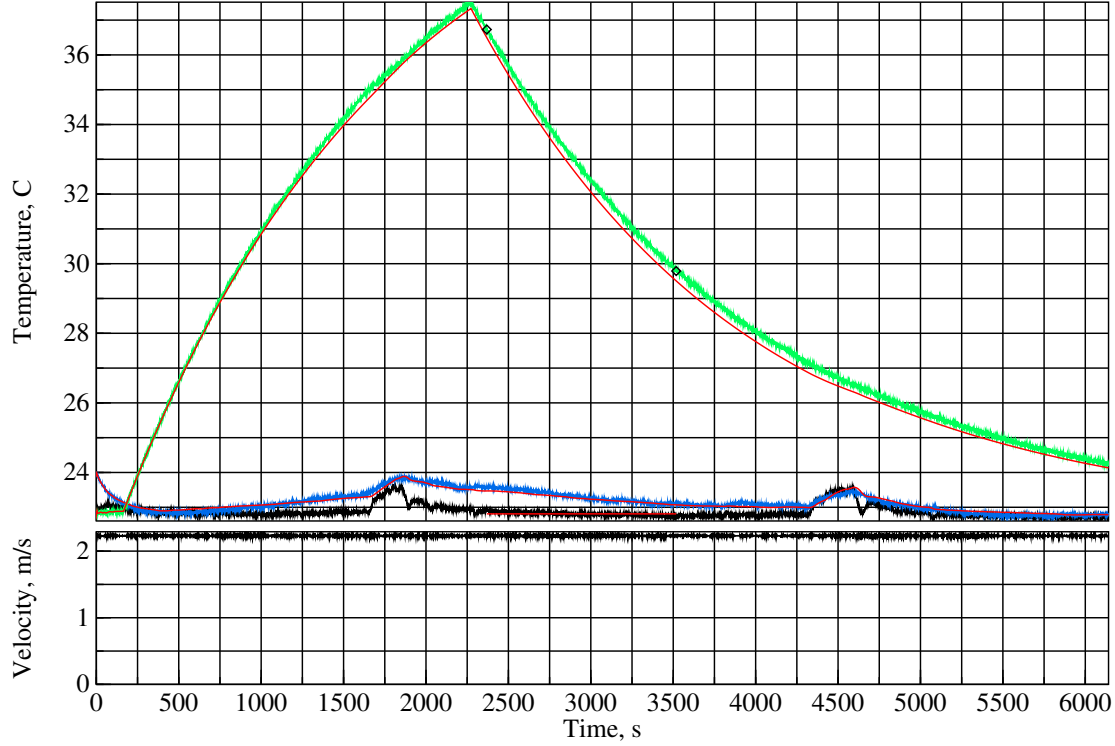

Estimated measurement uncertainties, bi-level 3mm roughness at $Re = 44536$.

Symbol	Nominal	Sensitivity	Bias	Uncertainty	Component
ΔT	10.1K	+10.8%/K	0.10K	1.08%	LM35C differential
P	101kPa	+0.0009%/Pa	1.5kPa	1.36%	MPXH6115A6U air pressure
C_{pt}	4.69kJ/K	+0.023%/(J/K)	47J/K	1.07%	plate thermal capacity
η	0.409	+205%	0.014	2.94%	anemometer calibration
C_S	1.000	-6.81%	0.050	0.34%	side reuptake
C_B	1.000	-2.56%	0.100	0.26%	back reuptake
ς	6.00mm	+8979%/m	100um	0.90%	post height
ϵ_{wt}	0.900	+8.62%	0.025	0.22%	wind-tunnel emissivity
				3.74%	combined bias uncertainty
Symbol	Nominal	Sensitivity	Variability	Uncertainty	Component
ω	640r/min	+0.132%/(r/min)	4.8r/min	0.63%	fan rotation rate
				3.95%	RSS combined uncertainty


20160828T040504Z – mixed Convection – Roughness=3.00mm; T=23.4+10.0°C; -90.00°
905±4.1r/min, V=3.0m/s, Re=60874, Ra/L^3=0.944x10^9, h=36.4W/(K.m^2), U=3.38W/K, Nu=428.8

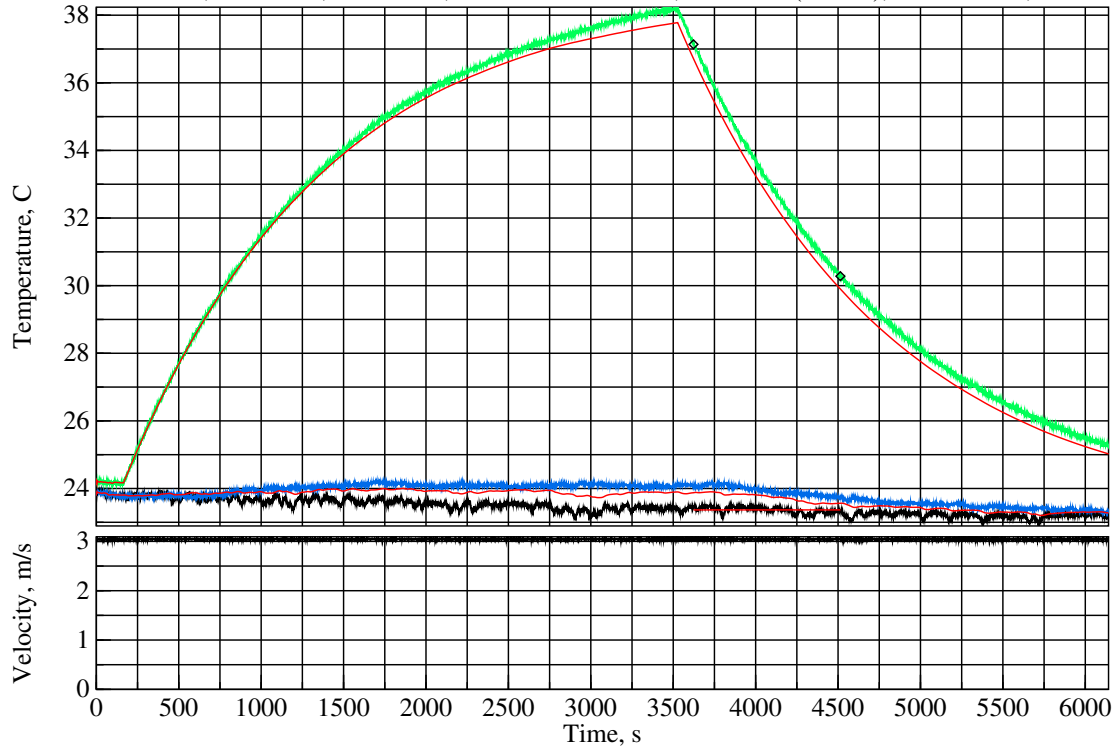

Estimated measurement uncertainties, bi-level 3mm roughness at $Re = 60875$.

Symbol	Nominal	Sensitivity	Bias	Uncertainty	Component
ΔT	9.97K	+10.7%/K	0.10K	1.07%	LM35C differential
P	102kPa	+0.0008%/Pa	1.5kPa	1.23%	MPXH6115A6U air pressure
C_{pt}	4.69kJ/K	+0.023%/(J/K)	47J/K	1.06%	plate thermal capacity
η	0.409	+173%	0.014	2.48%	anemometer calibration
C_S	1.000	-5.18%	0.050	0.26%	side reuptake
ς	6.00mm	+11316%/m	100um	1.13%	post height
				3.38%	combined bias uncertainty
Symbol	Nominal	Sensitivity	Variability	Uncertainty	Component
ω	905r/min	+0.080%/(r/min)	4.1r/min	0.33%	fan rotation rate
				3.45%	RSS combined uncertainty


20160828T141201Z – mixed Convection – Roughness=3.00mm; T=22.8+07.9°C; –90.00°
1280±5.3r/min, V=4.1m/s, Re=82189, Ra/L^3=0.767x10^9, h=45.7W/(K.m^2), U=4.25W/K, Nu=539.7

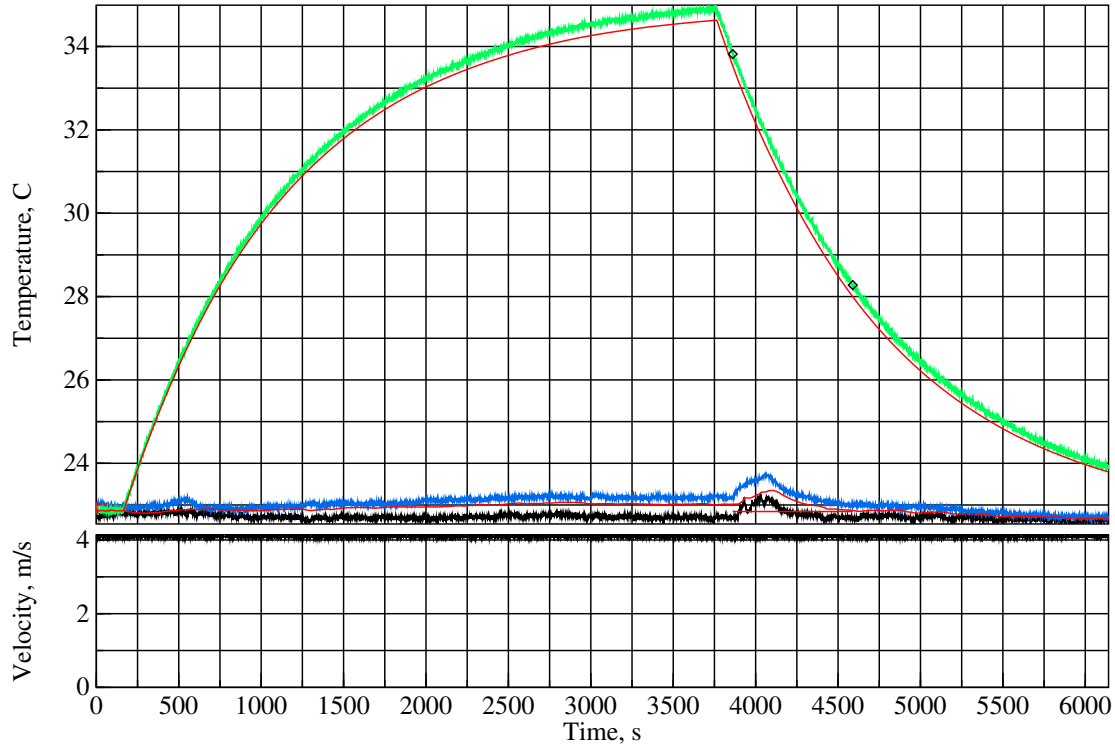

Estimated measurement uncertainties, bi-level 3mm roughness at $Re = 82184$.

Symbol	Nominal	Sensitivity	Bias	Uncertainty	Component
ΔT	7.91K	+13.3%/K	0.10K	1.33%	LM35C differential
P	102kPa	+0.0008%/Pa	1.5kPa	1.13%	MPXH6115A6U air pressure
C_{pt}	4.69kJ/K	+0.022%/(J/K)	47J/K	1.05%	plate thermal capacity
η	0.409	+138%	0.014	1.97%	anemometer calibration
u_u	7.943	+2.56%	0.100	0.26%	diffuser airflow upper bound
ς	6.00mm	+12428%/m	100um	1.24%	post height
				3.13%	combined bias uncertainty
Symbol	Nominal	Sensitivity	Variability	Uncertainty	Component
ω	1.28kr/min	+0.052%/(r/min)	5.3r/min	0.27%	fan rotation rate
				3.18%	RSS combined uncertainty

20160828T231631Z – mixed Convection – Roughness=3.00mm; T=22.6+07.6°C; -90.00°
1400±7.3r/min, V=4.4m/s, Re=88764, Ra/L^3=0.731x10^9, h=49.0W/(K.m^2), U=4.56W/K, Nu=578.9

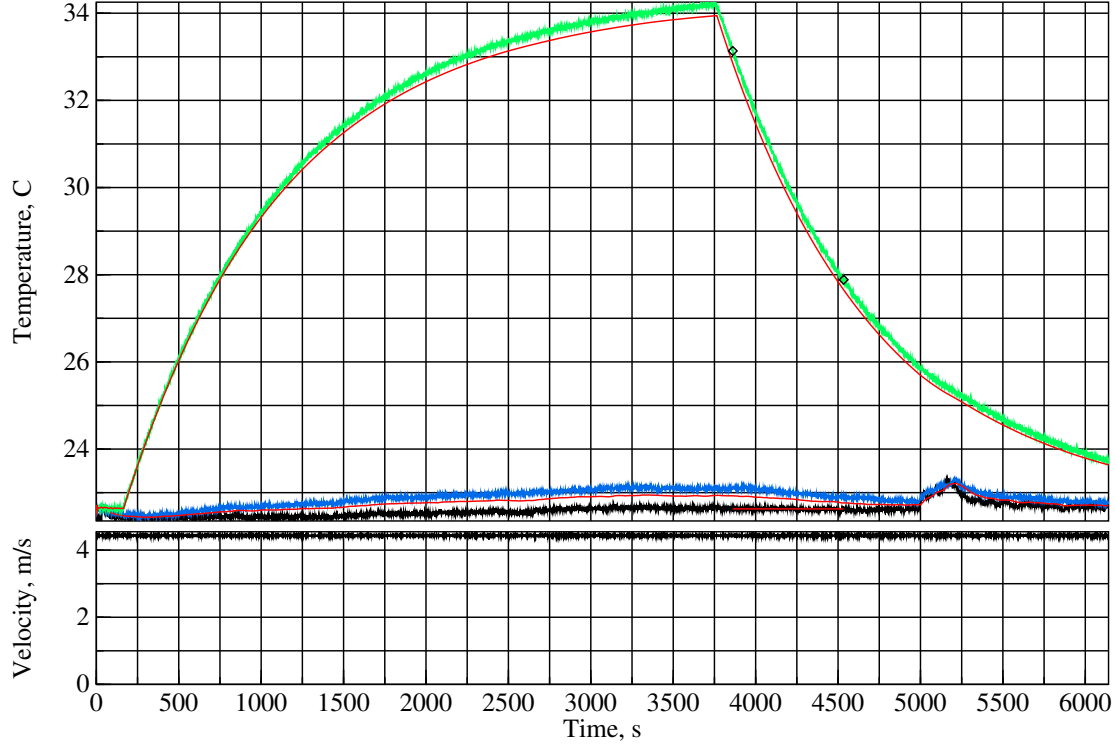

Estimated measurement uncertainties, bi-level 3mm roughness at $Re = 88775$.

Symbol	Nominal	Sensitivity	Bias	Uncertainty	Component
ΔT	7.57K	+13.9%/K	0.10K	1.39%	LM35C differential
P	101kPa	+0.0007%/Pa	1.5kPa	1.12%	MPXH6115A6U air pressure
C_{pt}	4.69kJ/K	+0.022%/(J/K)	47J/K	1.04%	plate thermal capacity
η	0.409	+127%	0.014	1.83%	anemometer calibration
u_u	7.943	+2.97%	0.100	0.30%	diffuser airflow upper bound
ς	6.00mm	+12428%/m	100um	1.24%	post height
				3.07%	combined bias uncertainty
Symbol	Nominal	Sensitivity	Variability	Uncertainty	Component
ω	1.40kr/min	+0.051%/(r/min)	7.3r/min	0.37%	fan rotation rate
				3.16%	RSS combined uncertainty